

# Medtronic


WE BRING  
FULLY ENABLED  
PROCEDURES  
TO YOUR OR.

#### Rialto™ SI Fusion System Indication

This device is intended for sacroiliac joint fusion for conditions including sacroiliac joint disruptions and degenerative sacroiliitis. Autograft and/or allograft may be placed in conjunction with the system.

Note: migration, loosening, or fracture of the implant may occur.


## Rialto™ SI Fusion System

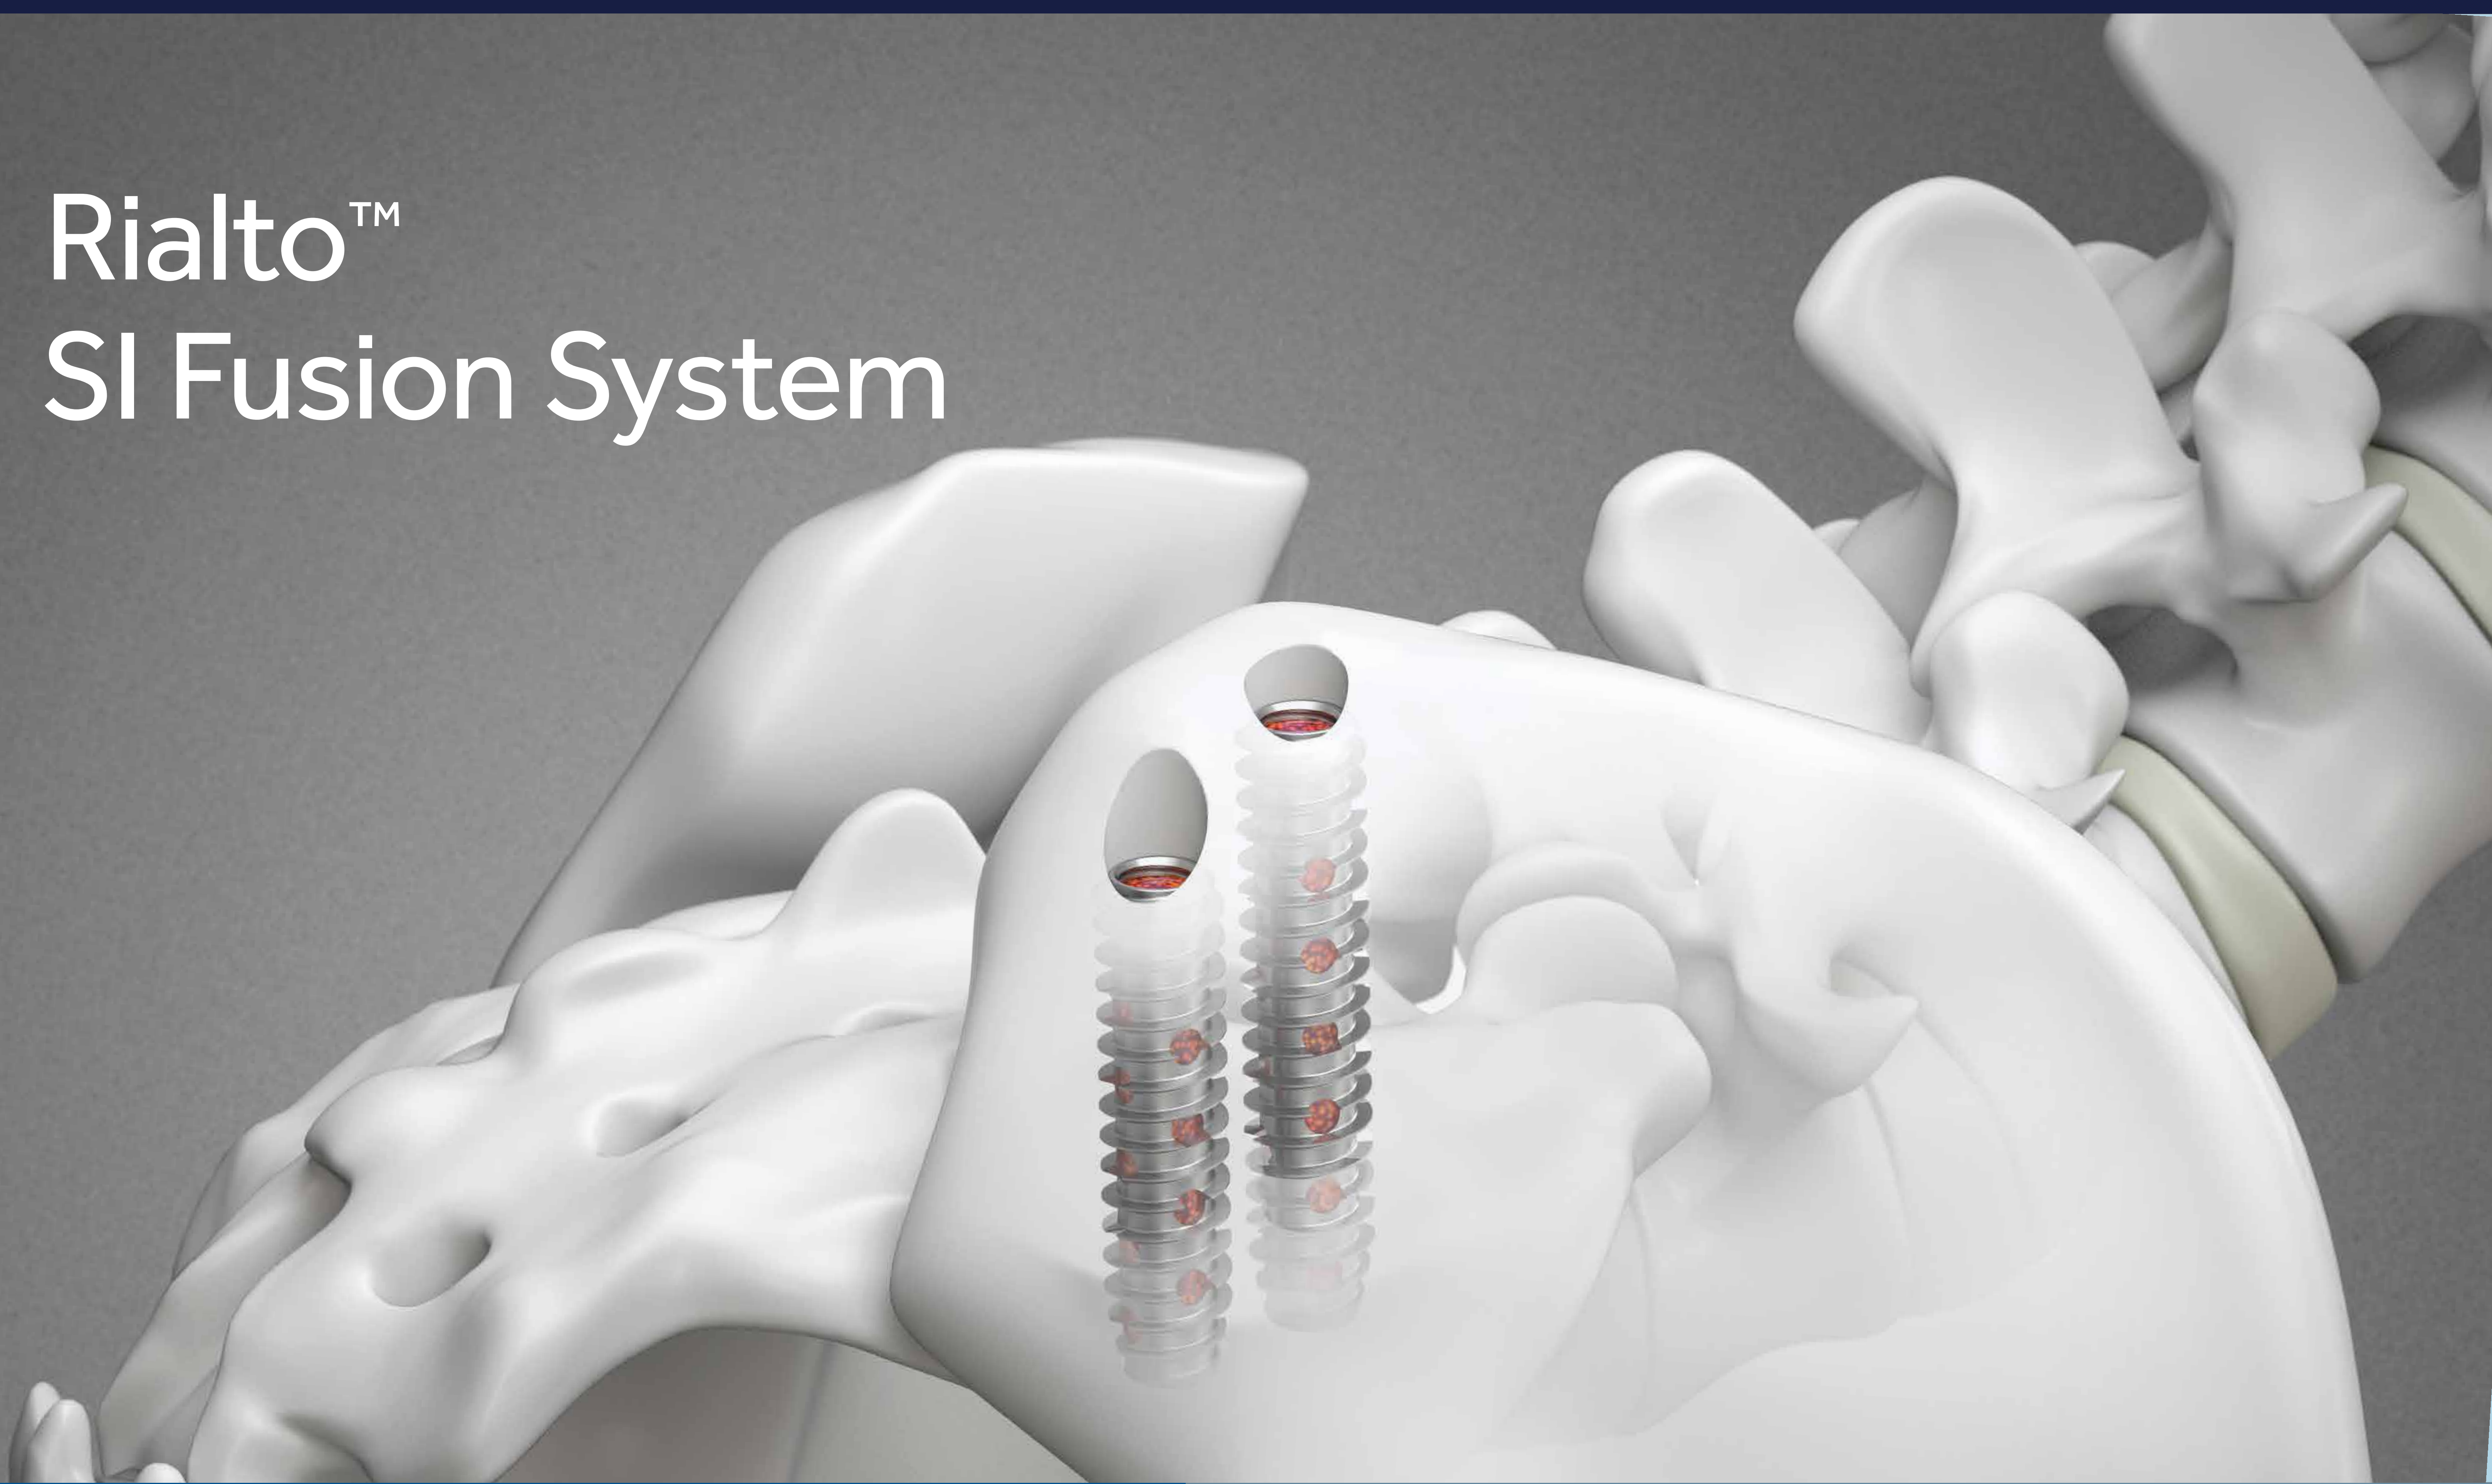

### O-Arm™ Imaging System



### StealthStation™ S7™ Navigation System

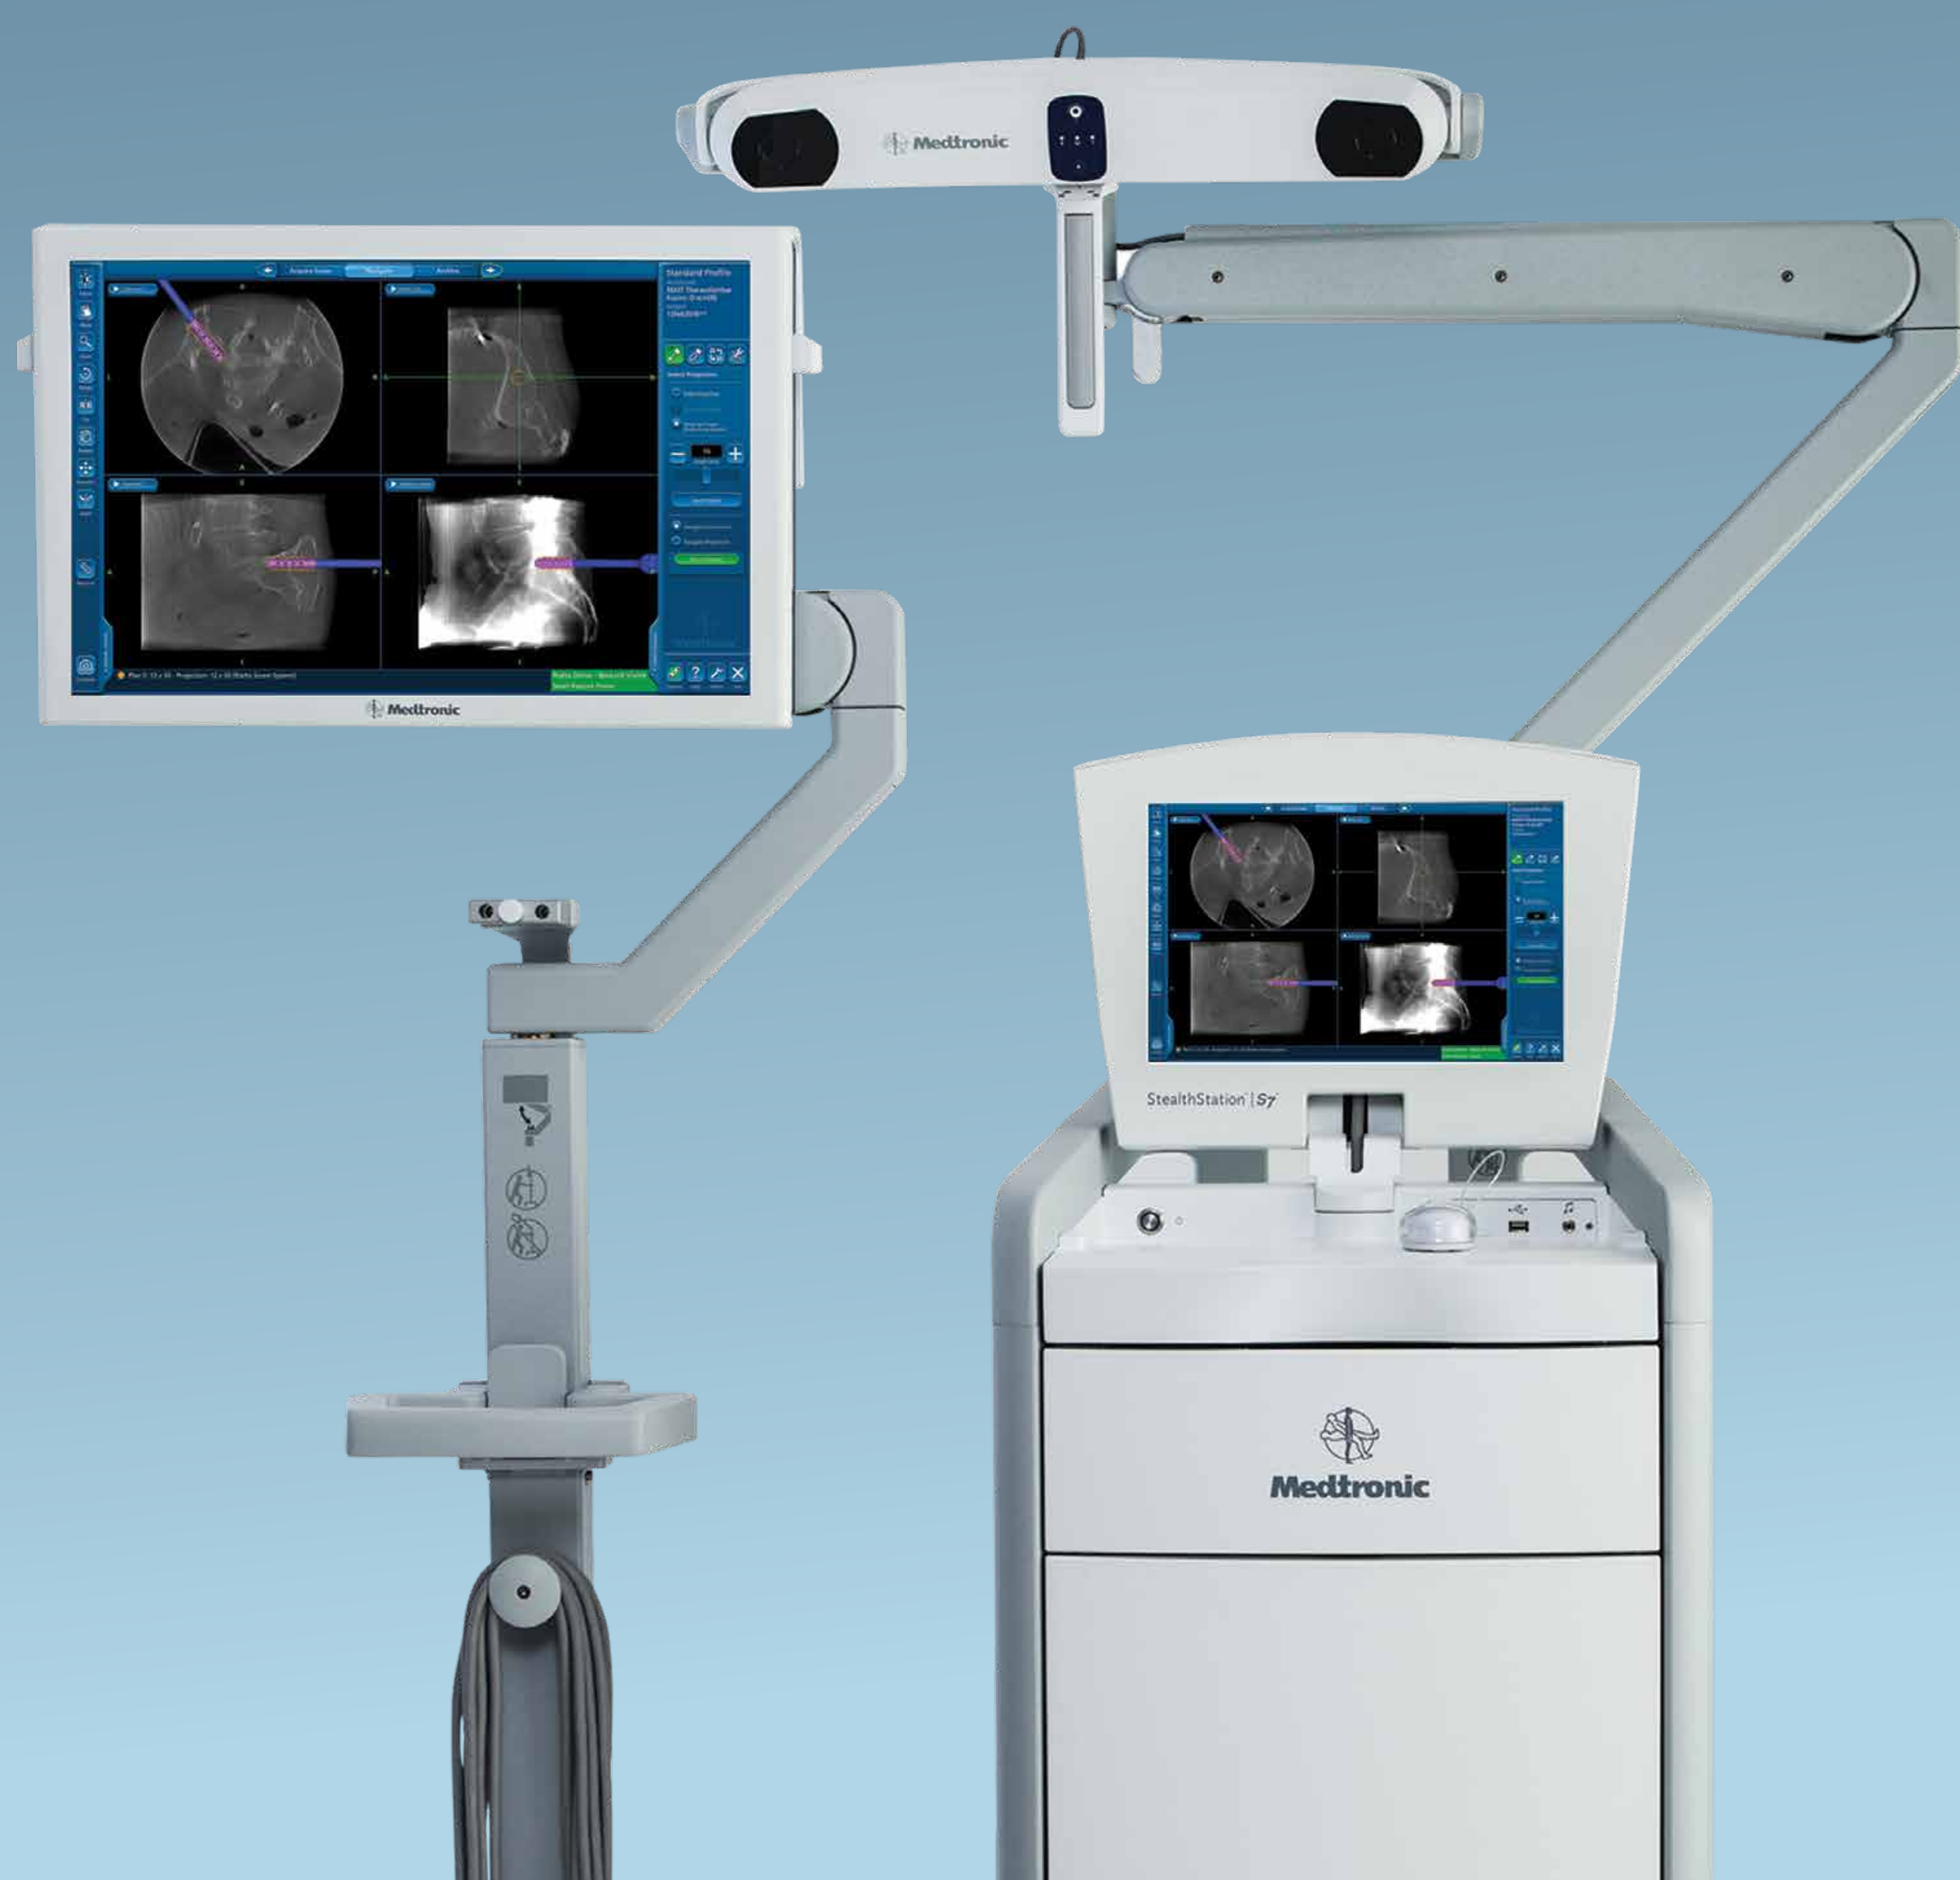

### Grafton™ Demineralized Bone Matrix (DBM) Putty



#### Grafton DBM DBF Indication & Risks:

Grafton DBM DBF can be used in orthopedic or reconstructive bone grafting procedures. The product can also be used in bone grafting procedures in combination with autologous bone or other forms of allograft bone, or alone as a bone graft. The presence of infection at the transplantation site is a contraindication for the use of this allograft. CAUTION: This allograft may contain trace amounts of gentamicin.

### IPC™ Powerease™ System



PMD018410-1.0 32628 UC201703812 EN

Leader, non-visual